



**Order #: COKAL0410AS**

## Soy

Soybean (*Glycine max*) is a legume which has been used for thousands of years as a food. Soybean is highly nutritious and is composed of 39% protein, some of which are allergens, such as Gly m3, Gly m4, Glycinin and Trypsin-inhibitor.

Soy products are widely used in the food industry, namely as texturizers, emulsifiers and protein fillers. People allergic to soy must strictly avoid the consumption of soy containing-food products. Cross contamination during the production process often occurs and soy residues in food cannot be excluded, thus sensitive detection systems are required.

## Short instructions



Perform extraction for finished product, rinse water or swab.




Transfer **12 drops** of extract to incubation vial.



Shake incubation vial vigorously by hand for **15 seconds**.



Incubate for **5 minutes** at room temperature.



Insert test strip into the solution and incubate for **5 minutes**.  
**Read result immediately.**

## Performance Characteristics:


**LOD:** 2 ppm Soy\* (Finished product & rinse water testing)  
2 µg/25cm<sup>2</sup> Soy\*\* (Swab testing)

\* LOD was determined in extraction solution


\*\* LOD was calculated

## Sample preparation – Finished Products and Rinse Water


**1. Homogenize** the sample (i.e. blend, crush, grind)




**2. Add 0.2 mL** Rinse water or **0.2g** of sample (weigh with Balance or estimate by filling up one of the extraction tube caps) to the sample extraction tube

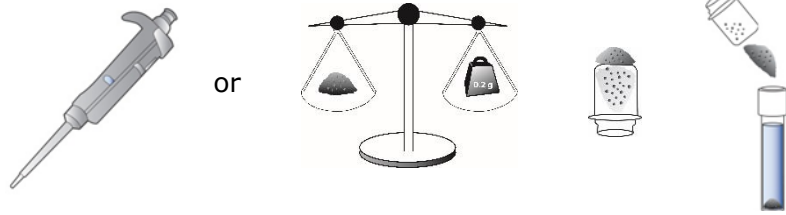


**3. Fill Extraction Tube with Extraction Buffer** to level shown below (blue arrow)



**4. Close tube with tube cap, and shake vigorously by hand for 1 minute.**




**5. Remove cap from the Extraction Tube and replace with dropper tip. And transfer 12 drops (400µl) to an incubation vial.**

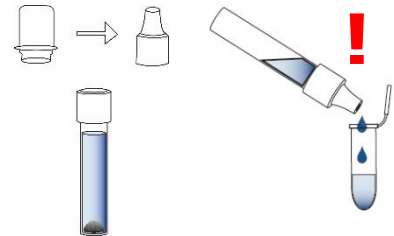


**Proceed to the Assay Section (page 3) to complete your test**

## Sample preparation – Swab Testing

**1. Fill extraction tube with Extraction Buffer** to level shown below (blue arrow), take a swab and wet the end by dipping into the buffer




**2. Wipe an area of 5cmx5cm** using side to side movements, rotating the swab tip as you go (we recommend the "cross-hatch" swabbing technique indicated below)

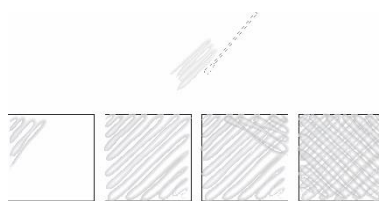

**3. Place the swab into the extraction tube. Carefully break off the end at the pre-scored point.**



**4. Close the tube with a cap and shake vigorously for 1 minute**



**5. Remove cap from the Extraction Tube and replace with dropper tip. And transfer 12 drops (400µl) to an incubation vial.**




**Proceed to the Assay Section (page 3) to complete your test**


## Assay Procedure in detail

---

**1.** Shake Incubation Vial vigorously by hand for **15 seconds** (ensuring liquid comes in contact with the lid of the vial) then leave to stand at room temperature for **5 minutes**.




**2.** Open the container of AgraStrips®, remove the necessary number of strips and close the tube. Open the Incubation Vial and insert the bottom end of test strip into the vial.



**3.** Remove the test strip from the Incubation Vial **after 5 minutes** and read the result immediately.

## Interpretation of Results

---

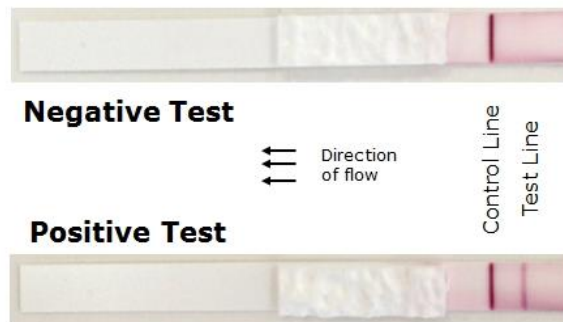

**One single purple line in the central part of the test = negative result**

(It is possible that the strip will turn pink during testing. In this case, the test line can appear as a white line on a pink background. This indicates a negative test result, and does not affect the performance of the test)

**Two purple lines in the result zone = positive result.** The sample contains allergen higher than the cut-off level and further investigations should be performed

**No control line appears = invalid result**, regardless of whether the test line appears. In the case of an invalid result, please repeat the procedure with a new strip. If the problem persists, please contact Romer Labs® before continuing further.

### **Important advice for the proper execution of the test:**

- It is important to **read the results immediately after the 5 minute incubate step** since the AgraStrip® test system has been validated extensively and shows reliable results after that exact time. Longer incubation times can lead to the development of false positive results.
- The AgraStrip® Allergen lateral flow tests are for the **detection of trace amounts of allergens** in a low ppm range. If the sample contains a lot of allergen (more than 1% but depending on the source of allergen), the test might come up negative.

## Performance Characteristics in Detail

---


**Limit of detection:** 2 ppm Soy (Finished product & rinse water testing)  
2 µg/25cm<sup>2</sup> Soy (Swab testing)

**Range of detection:** 2 – 1000000 ppm Soybean  
2 – 100000 ppm Soy protein Isolate  
2 – 30000 ppm Soymilk  
5000 – 500000 ppm Textured Soy Protein  
100000 – 1000000 ppm Soybean (roasted)

**pH range:** Performing the assay in a pH range of 6-8 will lead to reliable results. Highly acidic samples can lead to false positive results whereas in an alkaline milieu there is the tendency to false negative results.

## Materials Supplied with Kit:

---

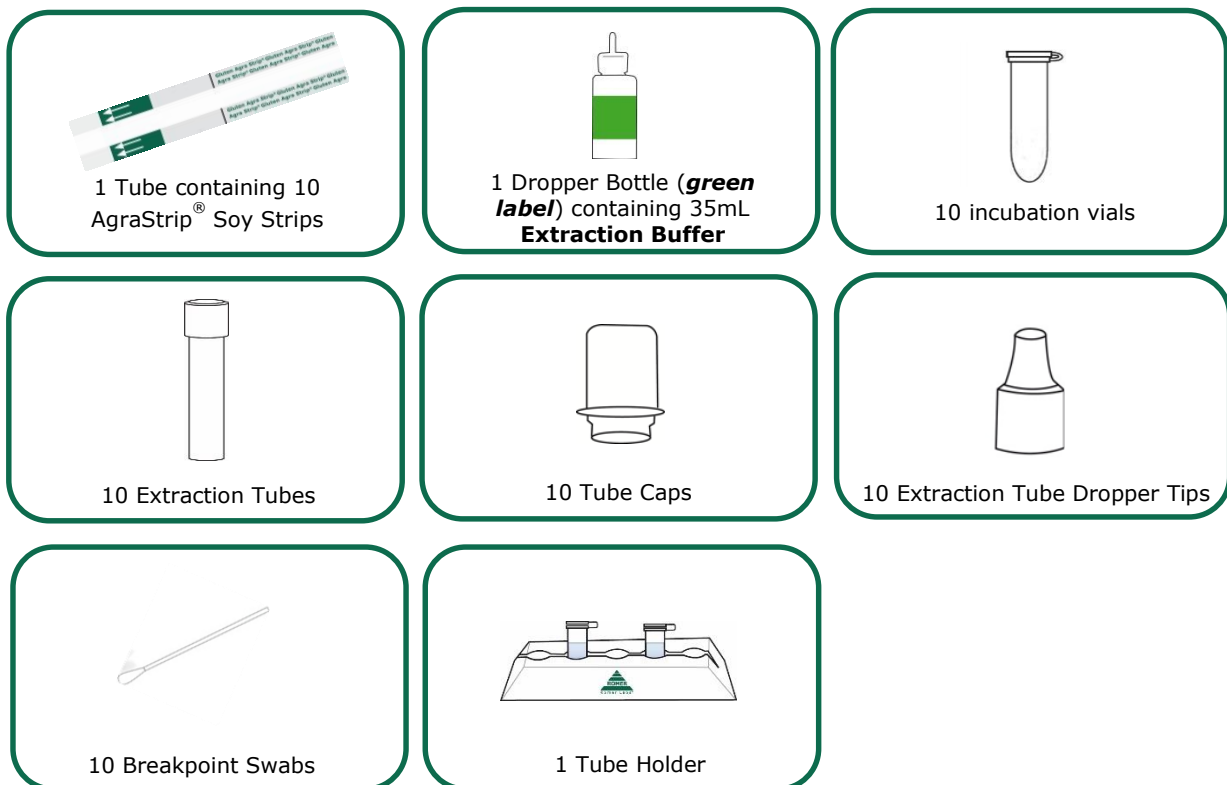

## Materials required but not supplied for solid sample preparation

---

- Blender or Crusher or Blade

## Technical and Background Information

---

The AgraStrip® Soy Test Kit is a lateral flow assay for the detection of Soy content in food, rinse waters and environmental swab samples.

### Soy Allergy

Soybean (*Glycine max*) is a legume which has been used for thousands of years as a food. Soybean is highly nutritious and is composed of 39% protein, some of which are allergens, such as Gly m3, Gly m4, Glycinin and Trypsin-inhibitor.

Soy products are widely used in the food industry, namely as texturizers, emulsifiers and protein fillers. People allergic to soy must strictly avoid the consumption of soy containing-food products. Cross contamination during the production process often occurs and soy residues in food cannot be excluded, thus sensitive detection systems are required.

### Assay Principles

Immunological rapid test in lateral flow format for the detection of Soy in food, rinse waters and swab samples (environmental samples). The extracted sample is transferred to an incubation vial that contains specific ready - to - use antibodies. If the sample contains Soy, an antigen-antibody complex will form. This is subsequently detected by the test strip. The test is easy to use, fast and reliable.

### Precautions

---

1. The product must be stored in its original package, between 15 and 25°C (room temperature). Do not use components beyond the expiration date indicated on the kit labels. Do not open the product until needed.
2. Test strips must be kept inside their original packaging, closed as tightly as possible. Do not freeze.
3. Adhere to the instructions for test procedures.
4. The components in this test kit have been quality control tested as a standard batch unit. Do not mix components from different lot numbers.

### Sampling:

Consideration must be taken that the food may contain an uneven distribution of Soy (spot contamination). It is important to test a representative portion of food as only a small amount of material is tested with the AgraStrip® Soy test.

### Detection:

The detection limit of the AgraStrip® Soy test is at the low ppm level but will vary depending on the food matrix being tested. To give reliable results each individual matrix should be validated before the kit is used routinely.


For further information regarding validation please contact Romer Labs.

### Note:

Chocolate and flour samples may block the filter tip of the extraction tube. This can be avoided by transferring the extract directly from the extraction tube to the reaction vial using a pipette or by hand to a level just under the 0.5ml graduation of the reaction vial



## Handling of the new improved AgraStrip® extraction buffer bottles

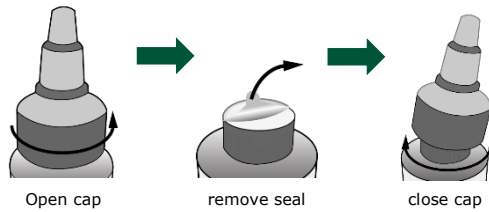

When opening the bottle for the 1<sup>st</sup> time, please take off the cap, peel off the seal and screw the cap back on the bottle.



To **open** the bottle just hold the neck of the upper part with your fingers and twist the corrugated screw top counterclockwise.

To **close** the bottle twist the screw top clockwise.

### For further information please contact:

Romer Labs UK Ltd.  
Block 5, The Heath Business &  
Technical Park,  
Runcorn, Cheshire, WA7 4QX

Tel: +44 (0) 845 519 50 10  
Email: [enquiry@romerlabs.com](mailto:enquiry@romerlabs.com)

### For customer service contact details in your country please visit:

[www.romerlabs.com](http://www.romerlabs.com)

### Warranty

The user assumes all risk in using Romer Labs UK Ltd products and services. Romer Labs UK Ltd will warrant that its products and services meet all quality control standards set by Romer Labs UK Ltd, and Romer Labs UK Ltd will, at its option, repair or replace any product, components, or repeat services which prove to be defective in workmanship or material within product specific warranty periods or expiration dates and which our examination shall disclose to our satisfaction to be defective as such. This warranty is expressly in lieu of all other warranties, expressed or implied, as to description, quality, merchantability, fitness for any particular purpose, productiveness, or any other matter. Romer Labs UK Ltd shall be in no way responsible for the proper use of its products. Romer Labs UK Ltd hereby disclaims all other remedies, warranties, guarantees or liabilities, expressed or implied, arising by law or otherwise, and it shall have no liability for any lost profits or damage, direct, indirect or otherwise, to person or property, in connection with the use of any of its products or services. This warranty shall not be extended, altered or varied except by a written instrument signed by an authorized representative of Romer Labs UK Ltd

Distribué par :

Z.A de Gesvrine - 4 rue Képler - B.P.4125  
44241 La Chapelle-sur-Erdre Cedex - France  
t. : +33 (0)2 40 93 53 53 | f. : +33 (0)2 40 93 41 00  
[commercial@humeau.com](mailto:commercial@humeau.com)



w w w . h u m e a u . c o m